

Allweighs Weighing Services
 Westend Grange
 West End Road
 Epworth
 Doncaster
 DN9 1LA
 Tel: 01427 875 867
 Web: www.allweighs.co.uk



Certificate No. JS:

2020683

Calibration Certificate of Accuracy

Business Name:

Address:

Contact Name:

Location:

Manufacturer:

Serial/Plant No:

Capacity:

Increment:

Frequency:

Test Date:

Next due:

Off-centre Loading:

Load point:	Reading:	Deviation:	Load point:	Reading:	Deviation:
1	6240	0	5	6240	0
2	6240	0	6	6240	0
3	6240	0			
4	6240	0			

Four loadcell

Six loadcell

	2		4		6
	1		3		5

Single loadcell

Eight loadcell

As Found

Measurement Points:	Reading:	Deviation:
0	0	0
8000	8000	0
16000	16000	0
23900	23900	0
33900	33900	0
43880	43860	20


Repeatability

43880	43880	0
-------	-------	---

Notes:

Engineer Name:

J Scott



Definitive

Measurement Points:	Reading:	Deviation:
0	0	0
8000	8000	0
16000	16000	0
23900	23900	0
33900	33900	0
43880	43880	0

Repeatability

43880	43880	0
-------	-------	---

Traceable Weights Used:

W20006 + 20007

Trading Standards Maximum Tolerance:

60


+/-

60

kg

Calibration method and equipment used traceable to national standards.

QMF17 Issue 5 14/07/2020



Allweighs Weighing Services
 Westend Grange
 West End Road
 Epworth
 Doncaster
 DN9 1LA
 Tel: 01427 875 867
 Web: www.allweighs.co.uk



Certificate No. JS:

2020685

Location: Out Weighbridge

Manufacturer: Dini Argeo

Serial/Plant No: 0100676301

Capacity: 50000 kg

Increment: 20 kg

Frequency: 12 months

Test Date: 5 November 2020

Next due: November 2021

Calibration Certificate of Accuracy

Business Name: Transwaste

Address: Gibson Lane
 Melton Industrial Estate
 North Ferriby
 Hull
 HU14 3HH

Contact Name: Leanne Swann

Off-centre Loading:

Load point:	Reading:	Deviation:	Load point:	Reading:	Deviation:
1	6240	0	5	6240	0
2	6220	20	6	6240	0
3	6240	0			
4	6220	20			

Four loadcell

Six loadcell

Single loadcell

Eight loadcell

As Found

Measurement Points:	Reading:	Deviation:
0	0	0
8000	8000	0
16000	16000	0
23900	23880	20
33900	33880	20
43880	43840	40

Repeatability

43880	43860	20
-------	-------	----

Notes: Weighbridge found to be within permitted tolerances.

Engineer Name:

J Scott

Definitive

Measurement Points:	Reading:	Deviation:
0	0	0
8000	8000	0
16000	16000	0
23900	23900	0
33900	33900	0
43880	43880	0

Repeatability

43880	43860	20
-------	-------	----

Traceable Weights Used:

W20006 + 20007

Trading Standards Maximum Tolerance:

60


+/-

60

kg

Calibration method and equipment used traceable to national standards.

QMF17 Issue 5 14/07/2020



Allweighs Weighing Services
 Westend Grange
 West End Road
 Epworth
 Doncaster
 DN9 1LA
 Tel: 01427 875 867
 Web: www.allweighs.co.uk



Certificate No. JS:

2020684

Location: In weighbridge

Manufacturer: Dini Argeo

Serial/Plant No: 0100659684

Capacity: 50000 kg

Increment: 20 kg

Frequency: 12 months

Test Date: 5 November 2020

Next due: November 2021

Calibration Certificate of Accuracy


Business Name: Transwaste

Address: Gibson Lane
 Melton Industrial Estate
 North Ferriby
 Hull
 HU14 3HH

Contact Name: Leanne Swann

Off-centre Loading:

Load point:	Reading:	Deviation:	Load point:	Reading:	Deviation:
1	6240	0	5	6240	0
2	6240	0	6	6220	20
3	6220	20			
4	6240	0			

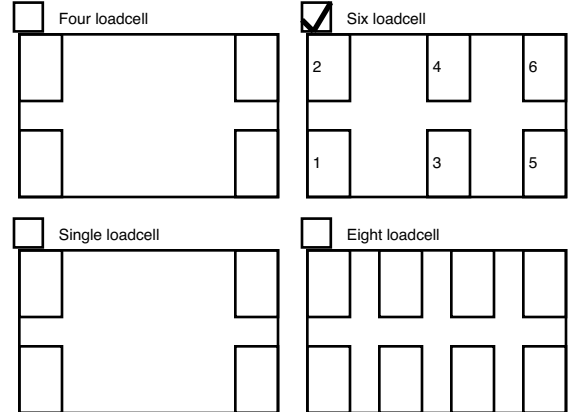

As Found

Measurement Points:	Reading:	Deviation:
0	0	0
8000	8000	0
16000	15980	20
23900	23880	20
33900	33869	40
43880	43820	60

Repeatability

43880	43860	20
-------	-------	----

Definitive

Measurement Points:	Reading:	Deviation:
0	0	0
8000	8000	0
16000	16000	0
23900	23900	0
33900	33900	0
43880	43860	20

Repeatability

43880	43880	0
-------	-------	---

Notes: Weighbridge found operating on tolerances, adjustments made.

Engineer Name:

J Scott

Traceable Weights Used:

W20006 + 20007

Trading Standards Maximum Tolerance:

60

+/-

60

kg

Calibration method and equipment used traceable to national standards.

QMF17 Issue 5 14/07/2020